

## Product Information

<b>Name</b>	Anti PIC monoclonal antibody
<b>Target</b>	plasmin- $\alpha$ 2-plasmininhibitor complex, PIC
<b>Target Species</b>	Human
<b>Target Description</b>	PIC is a 1:1 complex of $\alpha$ 2 plasmin inhibitor combined with plasmin, which can be used for diagnosis of fibrinolytic diseases.
<b>Host</b>	Mouse
<b>Product Description</b>	Monoclonal antibody produced by <i>in vitro</i> cell culture under conditions free from animal-derived components
<b>Conjugation</b>	Unconjugated/AP/AE/HRP
<b>Catalog #</b>	1021201/1021201(AP/AE/HRP)
<b>Solution</b>	Saline solution, pH 6.5-7.5 with preservative
<b>Appearance</b>	Clear, transparent liquid, colorless or slightly yellow
<b>Storage</b>	2-8°C
<b>Purity</b>	>95%
<b>Subclass</b>	IgG1, kappa
<b>Affinity (<math>K_{aff}</math>)</b>	$>10^9$ L/mol
<b>LoB</b>	User Guide
<b>Specificity</b>	Positive: / Negative: TM, TAT, tPAI-C, HSA
<b>Epitope</b>	ND
<b>Applications</b>	<input checked="" type="checkbox"/> ELISA <input checked="" type="checkbox"/> CLIA <input type="checkbox"/> GICA <input type="checkbox"/> FIA <input type="checkbox"/> IHC
<b>Pair</b>	<input type="checkbox"/> Capture <input checked="" type="checkbox"/> Detection
<b>Recommendations</b>	Pairable with #1021101
<b>Stability</b>	2 years
<b>Concentration</b>	2.0 mg/mL (+/-10%) or marked on the vial
<b>Lot #</b>	_____
<b>References</b>	

# User Guide

Catalog # 1021  
 Lot # \_\_\_\_\_

## CLIA

### Antigen Identification


The antigen adopted in the following assays is a widely recognized clinical applied product obtained commercially.

### Procedure

- Mix 20 $\mu$ L serially diluted antigen or serum samples with 20 $\mu$ L (diluted to working conc. 50T/mL) capture reagent of 1021101(B) and 20 $\mu$ L 0.6mg/mL streptavidin-conjugated magnetic beads. Incubate with stir at 37 $^{\circ}$ C for 30 minutes.
- Add 50 $\mu$ L (diluted to working conc. 20T/mL) detection reagent of 1021201(AP). Incubate with stir at 37 $^{\circ}$ C for 30 minutes.
- Measure the relative light unit (RLU) of each reaction with a clinical approved chemiluminescence analyzer.

### Measuring Range

The linear measuring range is 9-1111ng/mL ( $R^2>0.99$ ).

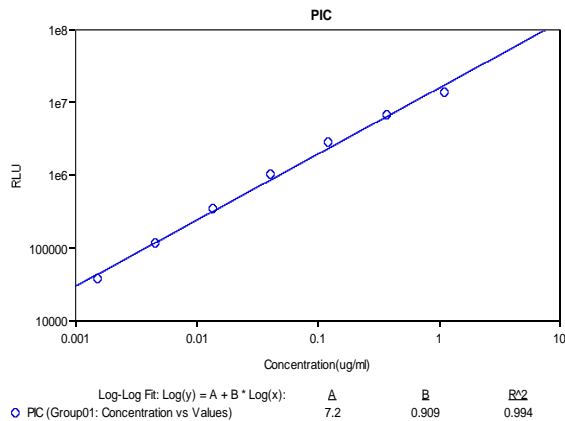

### Limit of Blank\* \*Follow the Guideline EP17 published by Clinical and Laboratory Standards Institute (CLSI)

Sample tested: blank samples. Tests: 20.

The LoB is 7ng/mL.

### Limit of Detection\* \*Follow the Guideline EP17 published by Clinical and Laboratory Standards Institute (CLSI)

Sample tested: low concentration samples. Tests: 20.

The LoD is 9ng/mL.

### Specificity

The assay shows no cross-reactivities when detecting antigens as follows: TAT at a tested conc. of 100ng/mL, TM at a tested conc. of 100ng/mL, tPAI-C at a tested conc. of 100ng/mL, human serum albumin at a tested conc. of 100mg/mL.

HKIG™ All Rights Reserved